

ISSN 1726-5479

SENSORS & TRANSDUCERS

vol. 95
8/08



Sensors and Transducers Applications

International Frequency Sensor Association Publishing



Editor-in-Chief: professor Sergey Y. Yurish, phone: +34 696067716, fax: +34 93 4011989,
e-mail: editor@sensorsportal.com

Editors for Western Europe

Meijer, Gerard C.M., Delft University of Technology, The Netherlands
Ferrari, Vittorio, Università di Brescia, Italy

Editors for North America

Datskos, Panos G., Oak Ridge National Laboratory, USA
Fabien, J. Josse, Marquette University, USA
Katz, Evgeny, Clarkson University, USA

Editor South America

Costa-Felix, Rodrigo, Inmetro, Brazil

Editor for Eastern Europe

Sachenko, Anatoly, Ternopil State Economic University, Ukraine

Editor for Asia

Ohyama, Shinji, Tokyo Institute of Technology, Japan

Editorial Advisory Board

- Abdul Rahim, Ruzairi**, Universiti Teknologi, Malaysia
Ahmad, Mohd Noor, Northern University of Engineering, Malaysia
Annamalai, Karthigeyan, National Institute of Advanced Industrial Science and Technology, Japan
Arcega, Francisco, University of Zaragoza, Spain
Arguel, Philippe, CNRS, France
Ahn, Jae-Pyoung, Korea Institute of Science and Technology, Korea
Arndt, Michael, Robert Bosch GmbH, Germany
Ascoli, Giorgio, George Mason University, USA
Atalay, Selcuk, Inonu University, Turkey
Atghiaee, Ahmad, University of Tehran, Iran
Augutis, Vyngantas, Kaunas University of Technology, Lithuania
Avachit, Patil Lalchand, North Maharashtra University, India
Ayesh, Aladdin, De Montfort University, UK
Bahreyni, Behraad, University of Manitoba, Canada
Baoxian, Ye, Zhengzhou University, China
Barford, Lee, Agilent Laboratories, USA
Barlingay, Ravindra, RF Arrays Systems, India
Basu, Sukumar, Jadavpur University, India
Beck, Stephen, University of Sheffield, UK
Ben Bouzid, Sihem, Institut National de Recherche Scientifique, Tunisia
Binnie, T. David, Napier University, UK
Bischoff, Gerlinde, Inst. Analytical Chemistry, Germany
Bodas, Dhananjay, IMTEK, Germany
Borges Carval, Nuno, Universidade de Aveiro, Portugal
Bousbia-Salah, Mounir, University of Annaba, Algeria
Bouvet, Marcel, CNRS – UPMC, France
Brudzewski, Kazimierz, Warsaw University of Technology, Poland
Cai, Chenxin, Nanjing Normal University, China
Cai, Qingyun, Hunan University, China
Campanella, Luigi, University La Sapienza, Italy
Carvalho, Vitor, Minho University, Portugal
Cecelja, Franjo, Brunel University, London, UK
Cerda Belmonte, Judith, Imperial College London, UK
Chakrabarty, Chandan Kumar, Universiti Tenaga Nasional, Malaysia
Chakravorty, Dipankar, Association for the Cultivation of Science, India
Changhai, Ru, Harbin Engineering University, China
Chaudhari, Gajanan, Shri Shivaji Science College, India
Chen, Jiming, Zhejiang University, China
Chen, Rongshun, National Tsing Hua University, Taiwan
Cheng, Kuo-Sheng, National Cheng Kung University, Taiwan
Chiriac, Horia, National Institute of Research and Development, Romania
Chowdhuri, Arijit, University of Delhi, India
Chung, Wen-Yaw, Chung Yuan Christian University, Taiwan
Corres, Jesus, Universidad Publica de Navarra, Spain
Cortes, Camilo A., Universidad Nacional de Colombia, Colombia
Courtois, Christian, Université de Valenciennes, France
Cusano, Andrea, University of Sannio, Italy
D'Amico, Arnaldo, Università di Tor Vergata, Italy
De Stefano, Luca, Institute for Microelectronics and Microsystem, Italy
Deshmukh, Kiran, Shri Shivaji Mahavidyalaya, Barshi, India
Dickert, Franz L., Vienna University, Austria
Dieguez, Angel, University of Barcelona, Spain
Dimitropoulos, Panos, University of Thessaly, Greece
Ding Jian, Ning, Jiangsu University, China
Djordjevich, Alexander, City University of Hong Kong, Hong Kong
Ko, Sang Choon, Electronics and Telecommunications Research Institute,
Donato, Nicola, University of Messina, Italy
Donato, Patricio, Universidad de Mar del Plata, Argentina
Dong, Feng, Tianjin University, China
Drljaca, Predrag, Instersema Sensoric SA, Switzerland
Dubey, Venketesh, Bournemouth University, UK
Enderle, Stefan, University of Ulm and KTB Mechatronics GmbH, Germany
Erdem, Gursan K. Arzum, Ege University, Turkey
Erkmen, Aydan M., Middle East Technical University, Turkey
Estelle, Patrice, Insa Rennes, France
Estrada, Horacio, University of North Carolina, USA
Faiz, Adil, INSA Lyon, France
Fericean, Sorin, Balluff GmbH, Germany
Fernandes, Joana M., University of Porto, Portugal
Francioso, Luca, CNR-IMM Institute for Microelectronics and Microsystems, Italy
Francis, Laurent, University Catholique de Louvain, Belgium
Fu, Weiling, South-Western Hospital, Chongqing, China
Gaura, Elena, Coventry University, UK
Geng, Yanfeng, China University of Petroleum, China
Gole, James, Georgia Institute of Technology, USA
Gong, Hao, National University of Singapore, Singapore
Gonzalez de la Rosa, Juan Jose, University of Cadiz, Spain
Grael, Annette, Goteborg University, Sweden
Graff, Mason, The University of Texas at Arlington, USA
Guan, Shan, Eastman Kodak, USA
Guillet, Bruno, University of Caen, France
Guo, Zhen, New Jersey Institute of Technology, USA
Gupta, Narendra Kumar, Napier University, UK
Hadjiiloucas, Sillas, The University of Reading, UK
Hashsham, Syed, Michigan State University, USA
Hernandez, Alvaro, University of Alcalá, Spain
Hernandez, Wilmar, Universidad Politecnica de Madrid, Spain
Homentcovschi, Dorel, SUNY Binghamton, USA
Horstman, Tom, U.S. Automation Group, LLC, USA
Hsiai, Tzung (John), University of Southern California, USA
Huang, Jeng-Sheng, Chung Yuan Christian University, Taiwan
Huang, Star, National Tsing Hua University, Taiwan
Huang, Wei, PSG Design Center, USA
Hui, David, University of New Orleans, USA
Jaffrezic-Renault, Nicole, Ecole Centrale de Lyon, France
Jaime Calvo-Galleg, Jaime, Universidad de Salamanca, Spain
James, Daniel, Griffith University, Australia
Janting, Jakob, DELTA Danish Electronics, Denmark
Jiang, Liudi, University of Southampton, UK
Jiang, Wei, University of Virginia, USA
Jiao, Zheng, Shanghai University, China
John, Joachim, IMEC, Belgium
Kalach, Andrew, Voronezh Institute of Ministry of Interior, Russia
Kang, Moonho, Sunmoon University, Korea South
Kaniusas, Eugenijus, Vienna University of Technology, Austria
Katake, Anup, Texas A&M University, USA
Kausel, Wilfried, University of Music, Vienna, Austria
Kavasoglu, Nese, Mugla University, Turkey
Ke, Cathy, Tyndall National Institute, Ireland
Khan, Asif, Aligarh Muslim University, Aligarh, India
Kim, Min Young, Koh Young Technology, Inc., Korea South

Korea South

Kockar, Hakan, Balikesir University, Turkey

Kotulska, Malgorzata, Wroclaw University of Technology, Poland

Kratz, Henrik, Uppsala University, Sweden

Kumar, Arun, University of South Florida, USA

Kumar, Subodh, National Physical Laboratory, India

Kung, Chih-Hsien, Chang-Jung Christian University, Taiwan

Lacnjevac, Caslav, University of Belgrade, Serbia

Lay-Ekuakille, Aime, University of Lecce, Italy

Lee, Jang Myung, Pusan National University, Korea South

Lee, Jun Su, Amkor Technology, Inc. South Korea

Lei, Hua, National Starch and Chemical Company, USA

Li, Genxi, Nanjing University, China

Li, Hui, Shanghai Jiaotong University, China

Li, Xian-Fang, Central South University, China

Liang, Yuanchang, University of Washington, USA

Liawruangrath, Saisunee, Chiang Mai University, Thailand

Liew, Kim Meow, City University of Hong Kong, Hong Kong

Lin, Hermann, National Kaohsiung University, Taiwan

Lin, Paul, Cleveland State University, USA

Linderholm, Pontus, EPFL - Microsystems Laboratory, Switzerland

Liu, Aihua, University of Oklahoma, USA

Liu Changgeng, Louisiana State University, USA

Liu, Cheng-Hsien, National Tsing Hua University, Taiwan

Liu, Songqin, Southeast University, China

Lodeiro, Carlos, Universidade NOVA de Lisboa, Portugal

Lorenzo, Maria Encarnacio, Universidad Autonoma de Madrid, Spain

Lukaszewicz, Jerzy Pawel, Nicholas Copernicus University, Poland

Ma, Zhanfang, Northeast Normal University, China

Majstorovic, Vidosav, University of Belgrade, Serbia

Marquez, Alfredo, Centro de Investigacion en Materiales Avanzados, Mexico

Matay, Ladislav, Slovak Academy of Sciences, Slovakia

Mathur, Prafull, National Physical Laboratory, India

Maurya, D.K., Institute of Materials Research and Engineering, Singapore

Mekid, Samir, University of Manchester, UK

Melnyk, Ivan, Photon Control Inc., Canada

Mendes, Paulo, University of Minho, Portugal

Mennell, Julie, Northumbria University, UK

Mi, Bin, Boston Scientific Corporation, USA

Minas, Graca, University of Minho, Portugal

Moghavvemi, Mahmoud, University of Malaya, Malaysia

Mohammadi, Mohammad-Reza, University of Cambridge, UK

Molina Flores, Esteban, Benemérita Universidad Autónoma de Puebla, Mexico

Moradi, Majid, University of Kerman, Iran

Morello, Rosario, DIMET, University "Mediterranea" of Reggio Calabria, Italy

Mounir, Ben Ali, University of Sousse, Tunisia

Mukhopadhyay, Subhas, Massey University, New Zealand

Neelamegam, Periasamy, Sastra Deemed University, India

Neshkova, Milka, Bulgarian Academy of Sciences, Bulgaria

Oberhammer, Joachim, Royal Institute of Technology, Sweden

Ould Lahoucine, University of Guelma, Algeria

Pamidighanta, Sayanu, Bharat Electronics Limited (BEL), India

Pan, Jisheng, Institute of Materials Research & Engineering, Singapore

Park, Joon-Shik, Korea Electronics Technology Institute, Korea South

Penza, Michele, ENEA C.R., Italy

Pereira, Jose Miguel, Instituto Politecnico de Setebal, Portugal

Petsev, Dimiter, University of New Mexico, USA

Pogacnik, Lea, University of Ljubljana, Slovenia

Post, Michael, National Research Council, Canada

Prance, Robert, University of Sussex, UK

Prasad, Ambika, Gulbarga University, India

Prateepasen, Asa, Kingmoungut's University of Technology, Thailand

Pullini, Daniele, Centro Ricerche FIAT, Italy

Pumera, Martin, National Institute for Materials Science, Japan

Radhakrishnan, S., National Chemical Laboratory, Pune, India

Rajanna, K., Indian Institute of Science, India

Ramadan, Qasem, Institute of Microelectronics, Singapore

Rao, Basuthkar, Tata Inst. of Fundamental Research, India

Raouf, Kosai, Joseph Fourier University of Grenoble, France

Reig, Candid, University of Valencia, Spain

Restivo, Maria Teresa, University of Porto, Portugal

Robert, Michel, University Henri Poincare, France

Rezazadeh, Ghader, Urmia University, Iran

Royo, Santiago, Universitat Politècnica de Catalunya, Spain

Rodriguez, Angel, Universidad Politécnica de Catalunya, Spain

Rothberg, Steve, Loughborough University, UK

Sadana, Ajit, University of Mississippi, USA

Sadeghian Marnani, Hamed, TU Delft, The Netherlands

Sandacci, Serghei, Sensor Technology Ltd., UK

Sapozhnikova, Ksenia, D.I.Mendeleyev Institute for Metrology, Russia

Saxena, Vibha, Bbhha Atomic Research Centre, Mumbai, India

Schneider, John K., Ultra-Scan Corporation, USA

Seif, Selemani, Alabama A & M University, USA

Seifter, Achim, Los Alamos National Laboratory, USA

Sengupta, Deepak, Advance Bio-Photonics, India

Shearwood, Christopher, Nanyang Technological University, Singapore

Shin, Kyuho, Samsung Advanced Institute of Technology, Korea

Shmaliy, Yuriy, Kharkiv National University of Radio Electronics, Ukraine

Silva Girao, Pedro, Technical University of Lisbon, Portugal

Singh, V. R., National Physical Laboratory, India

Slomovitz, Daniel, UTE, Uruguay

Smith, Martin, Open University, UK

Soleymanpour, Ahmad, Damghan Basic Science University, Iran

Somani, Prakash R., Centre for Materials for Electronics Technol., India

Srinivas, Talabattula, Indian Institute of Science, Bangalore, India

Srivastava, Arvind K., Northwestern University, USA

Stefan-van Staden, Raluca-Ioana, University of Pretoria, South Africa

Sumriddetchka, Sarun, National Electronics and Computer Technology Center, Thailand

Sun, Chengliang, Polytechnic University, Hong-Kong

Sun, Dongming, Jilin University, China

Sun, Junhua, Beijing University of Aeronautics and Astronautics, China

Sun, Zhiqiang, Central South University, China

Suri, C. Raman, Institute of Microbial Technology, India

Sysoev, Victor, Saratov State Technical University, Russia

Szewczyk, Roman, Industrial Research Institute for Automation and Measurement, Poland

Tan, Ooi Kiang, Nanyang Technological University, Singapore,

Tang, Dianping, Southwest University, China

Tang, Jaw-Luen, National Chung Cheng University, Taiwan

Teker, Kasif, Frostburg State University, USA

Thumbavanam Pad, Kartik, Carnegie Mellon University, USA

Tian, Gui Yun, University of Newcastle, UK

Tsiantos, Vassilios, Technological Educational Institute of Kaval, Greece

Tsigara, Anna, National Hellenic Research Foundation, Greece

Twomey, Karen, University College Cork, Ireland

Valente, Antonio, University, Vila Real, - U.T.A.D., Portugal

Vasashta, Ashok, Marshall University, USA

Vazques, Carmen, Carlos III University in Madrid, Spain

Vieira, Manuela, Instituto Superior de Engenharia de Lisboa, Portugal

Vigna, Benedetto, STMicroelectronics, Italy

Vrba, Radimir, Brno University of Technology, Czech Republic

Wandelt, Barbara, Technical University of Lodz, Poland

Wang, Jiangping, Xi'an Shiyou University, China

Wang, Kedong, Beihang University, China

Wang, Liang, Advanced Micro Devices, USA

Wang, Mi, University of Leeds, UK

Wang, Shinn-Fwu, Ching Yun University, Taiwan

Wang, Wei-Chih, University of Washington, USA

Wang, Wensheng, University of Pennsylvania, USA

Watson, Steven, Center for NanoSpace Technologies Inc., USA

Weiping, Yan, Dalian University of Technology, China

Wells, Stephen, Southern Company Services, USA

Wolkenberg, Andrzej, Institute of Electron Technology, Poland

Woods, R. Clive, Louisiana State University, USA

Wu, DerHo, National Pingtung University of Science and Technology, Taiwan

Wu, Zhaoyang, Hunan University, China

Xiu Tao, Ge, Chuzhou University, China

Xu, Lisheng, The Chinese University of Hong Kong, Hong Kong

Xu, Tao, University of California, Irvine, USA

Yang, Dongfang, National Research Council, Canada

Yang, Wuqiang, The University of Manchester, UK

Ymeti, Aurel, University of Twente, Netherland

Yong Zhao, Northeastern University, China

Yu, Haihu, Wuhan University of Technology, China

Yuan, Yong, Massey University, New Zealand

Yufera Garcia, Alberto, Seville University, Spain

Zagnoni, Michele, University of Southampton, UK

Zeni, Luigi, Second University of Naples, Italy

Zhong, Haoxiang, Henan Normal University, China

Zhang, Minglong, Shanghai University, China

Zhang, Qintao, University of California at Berkeley, USA

Zhang, Weiping, Shanghai Jiao Tong University, China

Zhang, Wenming, Shanghai Jiao Tong University, China

Zhou, Zhi-Gang, Tsinghua University, China

Zorzano, Luis, Universidad de La Rioja, Spain

Zourob, Mohammed, University of Cambridge, UK

Contents

Volume 95
Issue 8
August 2008

www.sensorsportal.com

ISSN 1726-5479

Research Articles

| | |
|--|-----|
| Measurement Uncertainties in the Experimental Field <i>M. T. Restivo and C. Sousa</i> | 1 |
| Potential Applications of Optical Fiber Based Distributed Sensor in Different Environment <i>Deepika Yadav and A. K. Nadir</i> | 13 |
| Acoustic Wave Parameter Extraction with Application to Delay Line Modelling Using Finite Element Analysis <i>Ajay Tikka, Said Al-Sarawi and Derek Abbott</i> | 26 |
| Optical Tomography Imaging in Pneumatic Conveyor <i>Ruzairi Abdul Rahim and Chan Kok San</i> | 40 |
| Ultrasonic Obstruction Detection and Distance Measurement Using AVR Micro Controller <i>Satish Pandey, Dharmendra Mishra, Anchal Srivastava, Atul Srivastava, R. K. Shukla</i> | 49 |
| A Low-cost, PC Interfaced Multipurpose Temperature Controlling System <i>Tanmoy Maity, Amritesh Chatterjee, Sujay Chandra</i> | 58 |
| Comparative Performance of Two Fiber Optic Ammonia Sensors Employing Different Sensing Materials <i>Jinesh Mathew, V. V. Mahesh and P. Radhakrishnan</i> | 65 |
| Poly (vinyl chloride) Based Ion Selective Electrode for Determination of Zr (IV) Ions Based on 2, 6-Dibenzylidenecyclohexanone <i>Syed A. Nabi, Aabid H. Shalla</i> | 72 |
| Resistive Ammonia Gas Sensor Based on Non-stoichiometric Copper Sulfide Thin Films <i>Abhay A. Sagade and Ramphal Sharma, Rajaram S. Mane and Sung-Hwan Han</i> | 81 |
| PVC Based Membrane of Ti(IV) Iodovanadate for Pb(II) Determination <i>Mu. Naushad</i> | 86 |
| Electrochemical DNA Biosensor for Detection of Aqueous Toxicants <i>B. Kuswandi and F. Sevilla III</i> | 97 |
| Development of Portable Phonocardiographic Fetal Heart Rate Monitor <i>Jianfeng Chen, Koksoon Phua, Ying Song</i> | 108 |
| Model Based Tuning of Controller for an Aerobic System <i>J. Sumathi, S. Sundaram</i> | 128 |
| Photogrammetric Resection Approach Using Straight Line Features for Estimation of Cartosat-1 Platform Parameters <i>Nita H. Shah, B. Islam And B. Gopala Krishna</i> | 134 |

Authors are encouraged to submit article in MS Word (doc) and Acrobat (pdf) formats by e-mail: editor@sensorsportal.com
Please visit journal's webpage with preparation instructions: <http://www.sensorsportal.com/HTML/DIGEST/Submission.htm>



PVC Based Membrane of Ti(IV) Iodovanadate for Pb(II) Determination

Mu. Naushad

Chemistry Laboratory, Department of Chemistry, Faculty of Science & Humanities,
SRM University, Modinagar, India
Tel.: +91-9897830017
E-mail: shad81@rediffmail.com

Received: 19 June 2008 /Accepted: 15 August 2008 /Published: 25 August 2008

Abstract: Ti(IV) iodovanadate has been synthesized by mixing a mixture of aqueous solutions of 0.1 M sodium vanadate and 0.1 M potassium iodate with 0.1 M solution of Ti(IV) chloride at pH 1.0. Distribution coefficients (K_d) of various metal ions were determined on the column of Ti(IV) iodovanadate which showed the selectivity of Pb(II) ions by this cation exchange material. So Ti(IV) iodovanadate has been used as an electroactive material for the construction of Pb(II) selective electrode. The main purpose of this study is to develop an inexpensive, simple and reliable ion-selective electrode for Pb(II) determination. The sensor exhibit Nernstian response for Pb(II) ions over a wide concentration range of 1×10^{-7} M to 1×10^{-1} M with a slope of 30 ± 0.4 mV per decade of activity. The electrode is suitable for use in aqueous solution in a pH range of 2-7.2 with a response time of 10 second. The membrane electrode can be used at least for 4 months without any divergence in potential. The selectivity coefficients were determined by the mixed solution method and revealed that the electrode was selective for Pb(II) ions in the presence of interfering cations. The sensor could be used as an indicator electrode in the potentiometric titration of Pb(II) ions with EDTA. The practical applicability of the proposed sensor has been reported for Pb(II) determination in a standard rock sample and water sample. The results are found to be in good agreement with those obtained by using conventional methods. *Copyright © 2008 IFSA.*

Keywords: Lead ion-selective electrode, Ti(IV) iodovanadate, Pb(II), Poly (vinyl chloride)

1. Introduction

Over recent years, the need of controlling the level of environmental pollutants in natural waterways, portable water and soils has generated increasing interest in the development of novel sensors for the detection of heavy metals. Among the heavy metals, lead is the most commonly encountered toxic pollutant in the environment as a result of its use in batteries, gasoline, solder, pipes and paints. It is a serious poison and tends to accumulate in the bone structure when ingested in levels exceeding the natural elimination rate of about 300 $\mu\text{g Pb/day}$ [1]. Lead can damage to the nervous system and the kidneys. To monitor this type of metals in large number of environment samples, potentiometric detectors based on ion-selective electrodes are suited because they offer advantages such as high selectivity, sensitivity, fast response, good precision, simplicity and low cost [2, 3]. These methods make possible direct monitoring of activities of selected species without pretreatment. The use of ion-selective electrodes (ISEs) for the detection and determination of lead has received much interest and many ligands have been investigated as sensing agents in electrodes [4]. Dicyclohexano-18-crown-6, benzo-18-crown-6, 15-crown-5 and their alkoxy, alkyl and methyl ester derivatives have also been successfully used as electroactive materials to develop selective sensors for Pb(II) ions [5–7]. Piroxicam, tetrabenzyl pyrophosphate, pyridinecarboximide derivatives, porphyrins, calixarenes, etc., have also been used as electroactive materials in Pb(II) selective electrodes [8-19] which show narrow working concentration range, high response time and suffer interference from some metal ions. A literature survey revealed that a limited number of membrane sensors using inorganic ion exchangers have been developed and most of these suffer from poor selectivity [20]. In the present study, we have used Ti(IV) iodovanadate inorganic cation exchanger as a sensing material for the construction of Pb(II) ion-selective electrode. The present sensor offers the advantages of thermal stability, simplicity, sensitivity, low cost, reliability, fast response and long life. In addition, the proposed sensor has been used for the determination of Pb(II) in a standard rock sample and water sample.

2. Experimental

2.1. Reagents

Titanium chloride (99%, Riedael-de Haen, Germany), potassium iodate (Otto Chemie, Bombay, India), sodium vanadate (Otto Chemie, Bombay, India). All other chemicals and reagents used were of analytical reagent grade.

2.2. Instrumentation

A single electrode pH meter (Toshniwal, India), a UV–Vis spectrophotometer (Elico EI 301E, India), a water bath incubator shaker and a digital potentiometer (Equiptronics EQ 609, India) with silver-silver chloride electrode as reference electrode were used.

2.3. Synthesis of Ti(IV) Iodovanadate

Ti(IV) iodovanadate was synthesized by mixing a mixture of aqueous solutions of 0.1 M sodium vanadate and 0.1 M potassium iodate with 0.1 M solution of Ti(IV) chloride at pH 1.0. The gelatinous precipitates, so formed were allowed to stand for 24 hrs in the mother liquor. The supernatant liquid was removed and the precipitates were washed with demineralized water several times to remove excess reagents. The products were dried at $40 \pm 2^\circ\text{C}$ in an oven. The dried products were then kept in demineralized water for cracking and to obtain the particle of the size range $\sim 125 \mu\text{m}$. These were

converted to H^+ form by placing them in 1.0 M HNO_3 solution and washed with demineralized water to remove excess acid and finally dried at $40 \pm 2^\circ C$.

2.4. Sorption Studies

In order to get an idea of partition behavior of the exchanger towards the separation of metal ions of analytical interest, distribution coefficients (K_d) were determined in demineralized water, di-methyl formamide and formamide mediums (Table 1). A, 0.4 g exchanger in H^+ form was treated with 40 mL solution of metal ions in required solvent medium in a 100 mL Erlenmeyer flask. The mixture was shaken for 6 hrs at $25 \pm 2^\circ C$ in a temperature controlled incubator shaker. The amount of metal ions before and after adsorption was determined by titration against a standard solution of 0.01 M disodium salt of EDTA. The K_d values may be expressed as follows:

$$K_d = \frac{\text{milli equivalent of metal ions / gm of ion - exchanger}}{\text{milli equivalent of metal ions / mL of solution}}$$

$$K_d = \frac{I-F}{F} \times \frac{V}{M} \text{ mL g}^{-1}, \quad (1)$$

where I is the initial amount of the metal ion in the solution phase, F is final amount of metal ion in the solution phase after treatment with the exchanger, V is the volume of the solution (mL) and M, the amount of ion exchanger taken (g).

Table 1. Distribution Coefficient (K_d) of metal ions on Ti(IV) iodovanadate in different solvent systems.

| Metal ions | Deminralized water | Di-methyl formamide | Formamide |
|------------|--------------------|---------------------|-----------|
| Mg^{2+} | 208 | 240 | 220 |
| Ca^{2+} | 186 | 214 | 196 |
| Sr^{2+} | 168 | 196 | 196 |
| Ba^{2+} | 168 | 179 | 170 |
| Cr^{3+} | 410 | 520 | 493 |
| Fe^{3+} | 280 | 418 | 387 |
| Co^{2+} | 168 | 630 | 520 |
| Ni^{2+} | 162 | 680 | 610 |
| Zn^{2+} | 178 | 597 | 436 |
| Cd^{2+} | 192 | 423 | 382 |
| Hg^{2+} | 187 | 287 | 218 |
| Pb^{2+} | 2418 | 2612 | 2319 |
| Al^{3+} | 204 | 521 | 476 |
| Ce^{3+} | 180 | 423 | 382 |

2.5. Membrane Preparation

The membranes were prepared as suggested by Coetzee and Benson [21]. The electroactive material Ti(IV) iodovanadate cation exchanger was grinded to fine powder and different amounts of this was mixed thoroughly with a fixed amount of PVC and dissolved in 10 mL of tetrahydrofuran (THF). The mixtures were vigorously shaken and when the solution got viscous, it was poured in a dust free Pyrex glass circles and solutions were allowed to evaporate at room temperature. The mixing ratio of the ion exchanger was varied in order to obtain a composition, which gave the best performance. In this way three sheets of different thickness were prepared.

2.6. Conditioning and Characterization of Membrane

The physicochemical properties of the membrane viz- water content, porosity, thickness and swelling etc. were determined as described elsewhere [22] after conditioning the membrane.

For conditioning, the membranes were equilibrated with 1 M NaCl and a few mL of CH₃COONa to adjust the pH in the range 5-6.5 (to maintain acid present in the film).

To find out the water content, the conditioned membranes were first dipped in water to elute diffusible salts and blotted with whatmann filter paper to remove surface moisture and weighed the water content was calculated as

$$\% \text{ Total weight} = \frac{W_w - W_d}{W_w} \times 100, \quad (2)$$

where W_w is the weight of the wet membrane and W_d if the weight of dry membrane.

Porosity (ε) was determined as the volume of water incorporated in the cavities per unit membrane volume from the water content data:

$$\varepsilon = \frac{W_w - W_d}{AL\rho_w}, \quad (3)$$

where A is the area of the membrane, L is the thickness of the membrane and ρ_w is the density of water.

Membrane thickness was measured by taking the average thickness of the membrane by using screw gauze and the swelling was measured as the difference between the average thicknesses of the membrane before and after equilibration with 1M NaCl for 24 hrs. Composition of best performed membrane is listed in Table 2 along with their response characteristics.

2.7. Electrode Preparation

A transparent membrane of 5 mm. diameters was cut from master membrane and glued to one end of a Pyrex glass tube with the help of araldite. The glass tube was filled with a 0.1 M Pb(NO₃)₂ solution. Silver/ silver chloride electrodes were used as internal and external reference electrodes. All the potential measurements using the following cell were made at $25 \pm 0.5^\circ\text{C}$. The whole arrangement can be shown as

Internal reference electrode (Ag/AgCl) 3.0 M KCl Internal electrolyte, 0.1 M Pb²⁺ Membrane Sample solution 3.0 M KCl External reference electrode (AgCl/Ag)

The performance of the electrode was investigated by measuring the e.m.f. of Pb(II) ion solution over the pH range of 1×10^{-1} to 1×10^{-10} M. The membrane electrode was conditioned by soaking in a 0.1 M Pb(NO₃)₂ solution for 2 days and at least 1 hr before use. After performing the experiment, membrane electrode was removed from the test solution and kept in 0.1 M Pb(NO₃)₂. Potential measurement of the membrane electrode was plotted against the selected concentration of the respective ions in an aqueous medium using the electrode assembly. The calibration graphs were plotted three times to check the reproducibility of the system.

Table 2. Characterization of ion-exchanger membrane.

| S. No | Membrane composition | | Thickness (mm) | Water content as % weight of wet membrane | Porosity | Swelling as % wt of wet membrane | Working conc. Range (Molar) | Slope (± 0.4 mV/decade of activity) | Response time (sec.) |
|-------|----------------------|----------|----------------|---|----------|----------------------------------|--|--|----------------------|
| | TiV (mg) | PVC (mg) | | | | | | | |
| S-1 | 150 | 200 | 0.41 | 2.4 | 0.082 | 0.12 | 1.0×10^{-7} to 1.0×10^{-1} | 30 | 10 |
| S-2 | 250 | 200 | 0.68 | 10.5 | 0.384 | 0.15 | 1×10^{-6} to 1.0×10^{-1} | 34 | 18 |
| S-3 | 300 | 200 | 0.84 | 14.7 | 0.412 | 0.20 | 5.6×10^{-6} to 1.0×10^{-1} | 33 | 26 |

TiV-Ti(IV) iodovanadate

3. Results and Discussion

Ti(IV) iodovanadate was synthesized by mixing a mixture of aqueous solutions of 0.1 M sodium vanadate and 0.1 M potassium iodate with 0.1 M solution of Ti(IV) chloride at pH 1.0. In order to explore the potentiality of this new inorganic cation exchange material in the separation of metal ions, distribution studies of various metal ions have been performed in demineralized water, di-methyl formamide and formamide mediums (Table 1). The distribution studies of various metal ions showed the selectivity of Pb(II) ions by this cation exchange material. So Ti(IV) iodovanadate has been used as an electroactive material for the preparation of Pb(II) ion-selective membrane electrode. Three samples of Ti(IV) iodovanadate membrane were prepared using different mixing ratios of electroactive Ti(IV) iodovanadate with a fixed amount of PVC. These three membranes were characterized to find out the membrane of good electrochemical performance for the purpose of preparation of an ion-selective membrane electrode. It is clear from Table 2 that, as the amount of Ti(IV) iodovanadate increased the thickness, porosity, swelling and water content increased. Generally an ideal membrane should have less thickness, moderate swelling and water content capacity. Membrane S-1 which has minimum amount of Ti(IV) iodovanadate has low order of water content, swelling porosity, thickness and shows wide working concentration range and quick response. So membrane S-1 was selected for the preparation of ion selective electrode for detail studies.

3.1. Working Concentration Range and Slope

The electrode prepared from membrane sample S-1 shows response for the Pb(II) ions in the concentration range of 1×10^{-7} M to 1×10^{-1} M with an average slope of 30 ± 0.4 mV (Fig. 1). Thus the working concentration range was found to be 1×10^{-7} M to 1×10^{-1} M for Pb(II) ions. A calibration curve was made by measuring the electrode response to standard solution prepared by serial dilution method without the addition of extra indifferent salts.

3.2. Response Time and Lifetime of the Membrane Electrode

The response time of a membrane sensor is an important factor. The average time required for the electrode to reach a potential response was found 10 second as shown in Fig. 2. The membrane electrode could be used for at least 4 months without any measurable divergence in its response for Pb(II) ions. It is very important that the performance of any ion-selective electrode should be checked every time before using it for any analytical purpose. However the sensor was stored in 0.1 M Pb(II) solution during non-usage. Repeated monitoring of the potential on the same portion of the sample (1×10^{-3} M) gave a standard deviation of ± 1 mV and there was no significant change in the slope.

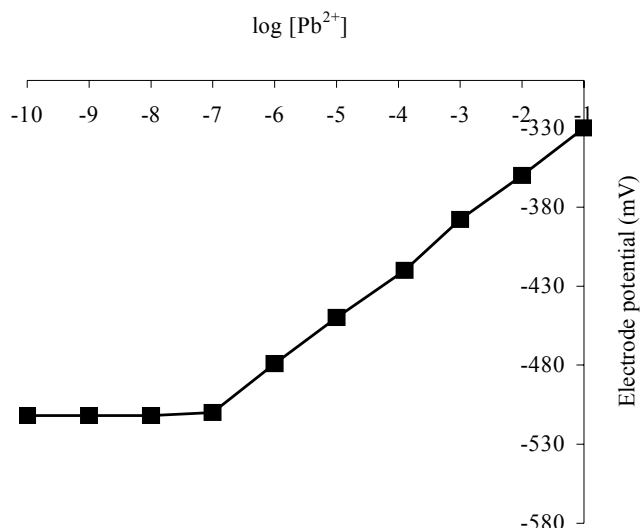


Fig. 1. Calibration curve for Ti(IV)iodovanadate membrane electrode in aqueous solution of Pb(NO₃)₂.

3.3. Effect of pH on the Test Solution

In order to determine the useful pH range over which the electrode can be used without any pH interference, the potential of the electrode was determined over a pH range of 1.0-8.0 (Fig. 3). pH was adjusted by drop wise addition of a 0.1 M solution of HNO₃ or NaOH and the e.m.f. of the electrode was measured at each pH value. It is clear from the figure that the potential remained constant in the pH range 2-7.2 which can be taken as the working pH range of the proposed sensor. Sharp change in potential values above pH 7.2 and below pH 2.0 may be due to the hydrolysis of Pb²⁺ ions and H⁺ ions interference, respectively [1].

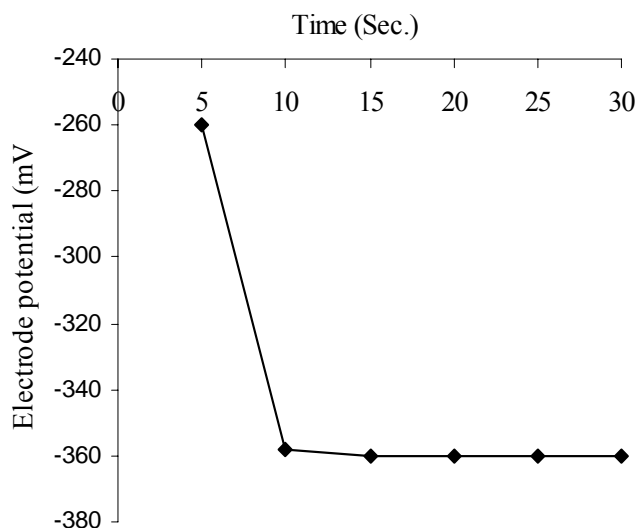


Fig. 2. Response of Pb(II) ion-selective Ti(IV) iodovanadate membrane electrode at different time interval.

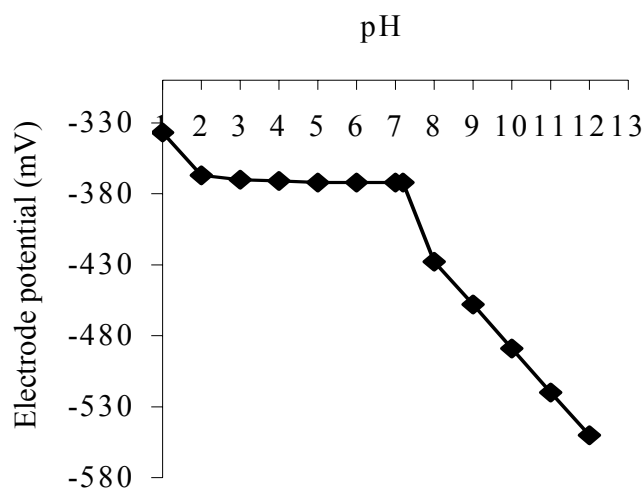


Fig. 3. Effect of pH on electrode response of Pb(II) ion-selective Ti(IV) iodovanadate membrane electrode.

3.4. Selectivity Coefficients

One of the important characteristics of any ion-selective electrode is its relative response to the primary ions over other ions present in the solution, which is termed as selectivity coefficient $K_{A,B}^{POT}$.

These were determined by the mixed solution method as discussed elsewhere [23]. A beaker of constant volume contained a mixed solution having a fixed concentration of interfering ion (M^{n+}) (1×10^{-3} M) and varying concentrations (1×10^{-1} to 1×10^{-10} M) of the primary ion. Now, the potential measurements were made by using the membrane electrode assembly and the results are summarized in Table 3. It is shown from the Fig. 4 that Mg^{2+} , Ca^{2+} , Sr^{2+} , Ba^{2+} , Hg^{2+} and Cd^{2+} ions do not interfere with the determination of Pb^{2+} ions and the interference due to Cr^{3+} , Al^{3+} , Fe^{3+} and Zn^{2+} is negligible. Ce^{3+} , Co^{2+} and Ni^{2+} register slight interference. Thus the results indicating that these interfering cations would not significantly disturb the functioning of Pb^{2+} ion-selective electrode and electrode is selective in the presence of these cations.

Table 3. Selectivity coefficients ($K_{Pb,M}^{POT}$) of various interfering ions for Pb^{2+} ion-selective electrode.

| Interfering ion (M^{n+}) | Selectivity coefficients ($K_{Pb,M}^{POT}$) |
|------------------------------|---|
| Hg^{2+} | 1×10^{-6} |
| Cr^{3+} | 1×10^{-6} |
| Fe^{3+} | 1×10^{-6} |
| Ni^{2+} | 1×10^{-5} |
| Co^{2+} | 1×10^{-5} |
| Zn^{2+} | 1×10^{-5} |
| Ce^{3+} | 1×10^{-5} |
| Cd^{2+} | 1×10^{-4} |
| Al^{3+} | 1×10^{-4} |

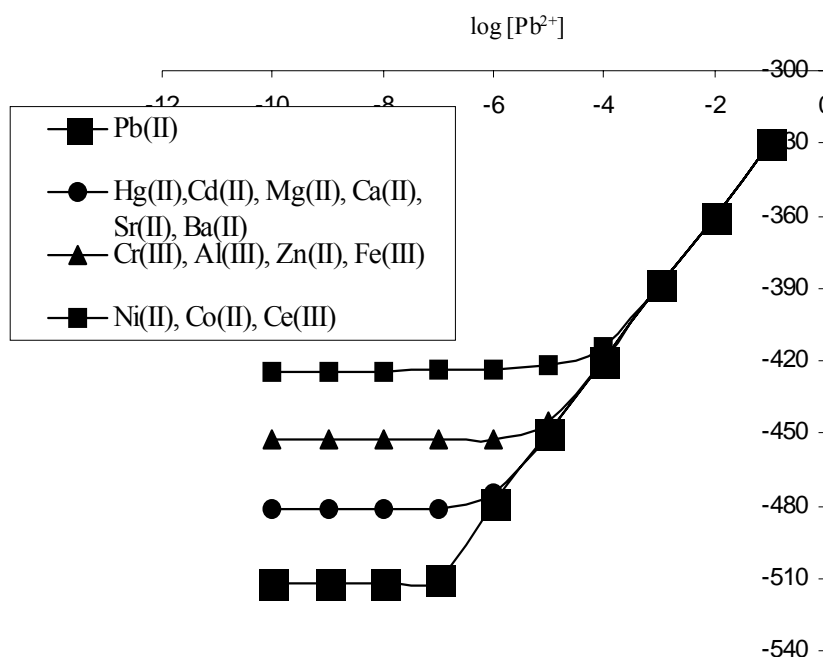


Fig. 4. Selectivity coefficients of various interfering ions for Ti(IV) iodovanadate-PVC membrane electrode.

A comparison of the present Pb^{2+} -ISEs with those already reported in the literature is given in Table 4. From Table 4, it is clear that the performance of the proposed $\text{Pb}(\text{II})$ ion-selective membrane electrode is comparable and better in many respects, such as the slope, response time, linear concentration range, life time, pH range and selectivity.

Table 4. Comparison of figure of merit of the present work with other studies.

| Sensor no. | Working concentration range (M) | Slope (mV/decade of activity) | pH range | Response time (s) | Detection limit (M) | Interference | Reference |
|------------|--|-------------------------------|----------|-------------------|-------------------------|--|-----------------|
| 1 | 5×10^{-5} to 1×10^{-2} | 28.3 | NR | 10 | 2.8×10^{-5} | Zn^{2+} , Ca^{2+} , Cd^{2+} , Ni^{2+} , K^{+} , Ag^{+} , Mn^{2+} , Tl^{+} , Li^{+} , NH_4^{+} , Sr^{2+} | 15 |
| 2 | 4×10^{-6} to 1×10^{-2} | 26-33.1 | 4.5-7 | 10 | 0.4-3.7 $\mu\text{g/L}$ | Ag^{+} , Cd^{2+} , Ca^{2+} , Hg^{2+} | 16 |
| 3 | 1×10^{-5} to 1×10^{-1} | 30 | 4-8 | 45 | $>4 \times 10^{-6}$ | Ag^{+} , Cu^{2+} | 20 |
| 4 | 2×10^{-6} to 1×10^{-2} | 29.3 | 3.5-6.3 | 45 | $>1.2 \times 10^{-6}$ | NR | 21 |
| 6 | 1×10^{-5} to 1×10^{-1} | 28 | 3-6 | 300 | $>1 \times 10^{-6}$ | K^{+} | 24 |
| 7 | 1×10^{-6} to 8×10^{-3} | 29 | 3-6 | 40 | $>8 \times 10^{-7}$ | Hg^{2+} | 25 |
| 8 | 1×10^{-7} to 1×10^{-1} | 31 | 2-6.0 | 25 | 1×10^{-7} | Cd^{2+} , Al^{3+} | Proposed sensor |

4. Analytical Applications

4.1. Determination of Pb(II) in Rock Sample

In order to test the analytical validity of this approach, the electrode has been used for the determination of lead in a standard rock sample (Mica shist (SDC-1), United States geological rock sample) and water sample. Two other techniques namely AAS, Uv-Vis spectrophotometer were also used for this purpose. The results obtained are presented in Table 5 and compared with those obtained by using AAS and Uv-Vis spectrophotometer. The sensor is found to be in satisfactory agreement with that obtained from atomic absorption spectrometer (AAS) and Uv-Vis spectrophotometer. These observations and results have been confirmed that present electrode can be used for practical analysis.

Table 5. Determination of Pb(II) in real samples using AAS, spectrophotometer and proposed sensor.

| Sample | Adjusted pH | AAS ($\mu\text{g} \times 10^{-4}$) | Spectrophotometer ($\mu\text{g} \times 10^{-4}$) | Proposed sensor ($\mu\text{g} \times 10^{-4}$) |
|--------------|-------------|--------------------------------------|--|--|
| Rock Sample | 5.0 | 3 \pm 0.02 | 2.4 \pm 0.05 | 2.6 \pm 0.04 |
| Water sample | 5.0 | 6 \pm 0.03 | 6.3 \pm 0.07 | 5.7 \pm 0.06 |

4.2. Potentiometric Titration

The analytical utility of this membrane electrode has been established by using it as an indicator electrode in the potentiometric titration of Pb^{2+} ions with an EDTA solution as a titrant (Fig. 5). A 10 mL of 1×10^{-3} solution of Pb^{2+} was titrated against 0.01 M EDTA solution at working pH of this electrode (5.0). The addition of EDTA causes a decrease in potential as a result of the decrease in free Pb^{2+} ion concentration due to the formation of Pb^{2+} -EDTA complex which give the idea of end point and therefore the proposed sensor can be used as an indicator electrode for the potentiometric determination of Pb^{2+} ions.

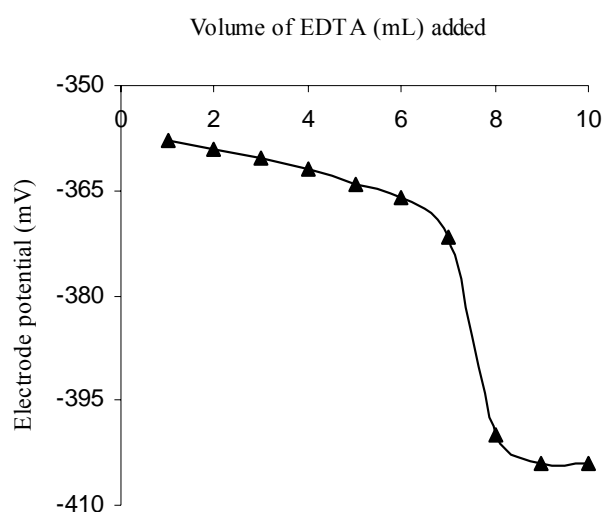


Fig. 5. Potentiometric titration of Pb(II) against EDTA solution.

5. Conclusion

In the present work, Ti(IV) iodovanadate has been used as an electroactive material for the preparation of Pb(II)-selective electrode. The membrane electrode has good operating characteristics such as sensitivity, stability and response time etc. The electrode could be used for Pb(II) determination in the concentration range of 1×10^{-7} M to 1×10^{-7} M at the functional pH range of 2-7.2. The sensor shows either comparable or better performance to the existing electrode already reported by many researchers for

Pb(II) determination regarding response characteristics (Table 4). The electrode could successfully be employed as indicator electrode in the potentiometric titration of Pb(II) against EDTA as well as to determine Pb(II) ions quantitatively in a standard rock sample.

Acknowledgement

The author is highly thankful to the Director, SRM-IMT, SRM University, Modinagar, for providing all necessary research facilities.

References

- [1]. V. K. Gupta, A. K. Jain, Pankaj Kumar, PVC-based membranes of *N, N'*-dibenzyl-1, 4, 10, 13-tetraoxa-7, 16-diazacyclooctadecane as Pb(II)-selective sensor, *Sensor and Actuators B*, 120, 2006, pp. 259-265.
- [2]. A. K. Covington, Ion-selective electrode methodology, Boca Raton FL, *CRC Press*, 2, 1979, p. 90.
- [3]. H. R. Zare, M. M. Ardakani, N. Nasirizadeh, J. Safari, Lead-selective poly(vinyl chloride) membrane electrode based on 1-phenyl-2-(2-quinolyl)-1, 2-dioxo-2-(4-bromo) phenylhydrazone, *Bull. Korean Chem. Soc.*, 26, 2005, pp. 51-56.
- [4]. P. Buhlmann, E. Pretsch, E. Bakker, Carrier-based ion-selective electrodes and bulk optodes. 2. Ionophores for potentiometric and optical sensors, *Chem. Rev.*, 98, 1998, pp. 1593-1687.
- [5]. E. Malinowska, J. Jurczak, T. Stankiewicz, Macrocyclic Oxamides as Ionophores for Lead-Selective Membrane Electrodes, *Electroanalysis*, 5, 1993, pp. 489-492.
- [6]. A. S. Attiyat, G. D. Christian, C. V. Cason, R. A. Bartsch, Benzo-18-crown-6 and Its Lariat Ether Derivatives as Ionophores for Potassium, Strontium, and Lead Ion-Selective Electrodes, *Electroanalysis*, 4, 1992, pp. 51-56.
- [7]. W. Hasse, B. Ahlers, J. Reinbold, K. Cammann, PbOH⁺-selective membrane electrode based on crown ethers, *Sens. Actuator B*, 19, 1994, pp. 383-386.
- [8]. M. M. Ardakany, A. A. Ensafi, H. Naeimi, A. Dastanpour, A. Shamlli, Highly selective lead(II) coated-wire electrode based on a new Schiff base, *Sens. Actuator B*, 96, 2003, pp. 441-445.
- [9]. J. Lu, R. Chen, X. He, A lead ion-selective electrode based on a calixarene carboxyphenyl azo derivative, *J. Electroanal. Chem.*, 528, 2002, pp. 33-38.
- [10]. S. Sadeghi, G. R. Dashti, M. Shamsipur, Lead-selective poly(vinyl chloride) membrane electrode based on piroxicam as a neutral carrier, *Sens. Actuator B*, 81, 2002, pp. 223-228.
- [11]. M. M. Zareh, A. K. Ghoneim, M. H. Abd El-Aziz, Effect of presence of 18-crown-6 on the response of 1-pyrrolidine dicarbodithioate-based lead selective electrode, *Talanta*, 54, 2001, pp. 1049-1057.
- [12]. M. F. Mousavi, S. Sahari, N. Alizadeh, M. Shamsipur, Lead ion-selective membrane electrode based on 1, 10-dibenzyl-1, 10-diaza-18-crown-6, *Anal. Chim. Acta*, 414, 2000, pp. 189-194.
- [13]. S. S. M. Hassan, M. H. Abou Ghalia, A. E. Amr, A. H. K. Mohamed, New lead (II) selective membrane potentiometric sensors based on chiral 2, 6-bis-pyridinecarboximide derivatives, *Talanta*, 60, 2003, pp. 81-91.
- [14]. H. K. Lee, K. Song, H. R. Seo, Y. Choi, S. Jean, Lead(II)-selective electrodes based on tetrakis (2-hydroxy-1-naphthyl)porphyrins: the effect of atropisomers, *Sens. Actuator B*, 99, 2004, pp. 323-329.
- [15]. T. Jeong, H. K. Lee, D. Jeong, S. Jeon, A lead(II)-selective PVC membrane based on a Schiff base complex of *N, N'*-bis(salicylidene)-2, 6-pyridinediamine, *Talanta*, 65, 2005, pp. 543-548.

- [16].V. S. Bhat, V. S. Ijeri, A. K. Srivastava, Coated wire lead(II) selective potentiometric sensor based on 4-*tert*-butylcalix[6].arene, *Sens. Actuator B*, 99, 2004, pp. 98-105.
- [17].S. Sadeghi, G. R. Dashti, M. Shamsipur, Lead-selective poly(vinyl cholride) membrane electrode based on piroxicam as a neutral carrier, *Sens. Actuator B*, 81, 2002, pp. 223-228.
- [18].A. Abbaspour, B. Khajeh, Lead(II)-Selective Electrode Based on Phenyl Disulfide, *Anal. Sci.*, 18, 2002, pp. 987-991.
- [19].A. K. Jain, V. K. Gupta, L. P. Singh, J. R. Raison, A comparative study of Pb²⁺ selective sensors based on derivatized tetrapyrazole and calix[4].arene receptors, *Electrochim. Acta*, 51, 2006, pp. 2547-2553.
- [20].C. J. Coetzee, *Ion-selective electrode Rev.*, 3, 1981, p. 105.
- [21].C. J. Coetzee, A. J. Benson, A cesium-sensitive electrode, *Anal. Chim. Acta*, 57, 1971, pp. 478-480.
- [22].S. Amarchand, S. K. Menon, Y. K. Agarwal, Rare-Earth Hydroxamate Complexes as Sensor Materials For Ion-Selective Electrodes, *Electroanalysis*, 12, 2000, pp. 522-527.
- [23].G. J. Moody, J. R. D. Thomas, *Selective Ion Sensitive Electrodes*, Watford, Merrow, 1971.
- [24].M. K. Jang, K. S. Ha, M. C. Soe, Coated Wire Lead(II) Ion-Selective Electrodes based on Crown Ethers, *J. Korean Chem. Soc.*, 41, 1997, pp. 337-341.
- [25].M. Shamsipur, M. R. Ganjali, A. Rouhollahi, Lead-Selective Membrane Potentiometric Sensor Based on an 18-Membered Thiacrown Derivative, *Anal. Sci.*, 17, 2001, pp. 935-942.

2008 Copyright ©, International Frequency Sensor Association (IFSA). All rights reserved.
(<http://www.sensorsportal.com>)

IDGA
Institute for Defense and
Government Advancement

7th Annual Light Armored Vehicles & Stryker™ Summit

November 17 – 20, 2008
Sheraton Premiere at
Tysons Corner, Vienna VA

www.LightArmoredVehiclesSummit.com

The home of the international LAV community returns to VA!

Guide for Contributors

Aims and Scope

Sensors & Transducers Journal (ISSN 1726-5479) provides an advanced forum for the science and technology of physical, chemical sensors and biosensors. It publishes state-of-the-art reviews, regular research and application specific papers, short notes, letters to Editor and sensors related books reviews as well as academic, practical and commercial information of interest to its readership. Because it is an open access, peer review international journal, papers rapidly published in *Sensors & Transducers Journal* will receive a very high publicity. The journal is published monthly as twelve issues per annual by International Frequency Association (IFSA). In addition, some special sponsored and conference issues published annually.

Topics Covered

Contributions are invited on all aspects of research, development and application of the science and technology of sensors, transducers and sensor instrumentations. Topics include, but are not restricted to:

- Physical, chemical and biosensors;
- Digital, frequency, period, duty-cycle, time interval, PWM, pulse number output sensors and transducers;
- Theory, principles, effects, design, standardization and modeling;
- Smart sensors and systems;
- Sensor instrumentation;
- Virtual instruments;
- Sensors interfaces, buses and networks;
- Signal processing;
- Frequency (period, duty-cycle)-to-digital converters, ADC;
- Technologies and materials;
- Nanosensors;
- Microsystems;
- Applications.

Submission of papers

Articles should be written in English. Authors are invited to submit by e-mail editor@sensorsportal.com 6-14 pages article (including abstract, illustrations (color or grayscale), photos and references) in both: MS Word (doc) and Acrobat (pdf) formats. Detailed preparation instructions, paper example and template of manuscript are available from the journal's webpage: <http://www.sensorsportal.com/HTML/DIGEST/Submission.htm> Authors must follow the instructions strictly when submitting their manuscripts.

Advertising Information

Advertising orders and enquires may be sent to sales@sensorsportal.com Please download also our media kit: http://www.sensorsportal.com/DOWNLOADS/Media_Kit_2008.pdf



Smart Sensors Systems Design

A five-day advanced engineering course
10-14 November 2008, Barcelona, Spain



General Information

This course is suitable for engineers who design different digital and intelligent sensors, data acquisition, and measurement systems. It is also useful for researchers, graduate and post graduate students. Course will be taught in English.

Course Description

An advanced engineering course describes modern developments and trends in the field of smart sensor systems and digital sensors design.

After a general overview of data acquisition methods, modern smart, digital and quasi-digital sensors, smart systems details are discussed. A systematic approach towards the design of low-cost high-performance smart sensors systems with self-adaptation and self-identification possibilities is presented.

Contact Person

Susana Escriche
Fundació UPC. Edifici Vèrtex
Plaça Eusebi Güell, 6, 08034 Barcelona
Tel.: +34 93 401 08 94
E-mail: susana.escriche@fundacio.upc.edu

Course Instructor

Prof. Sergey Y. Yurish,
Centre de Disseny d'Equips Industrials (CDEI),
Universitat Politècnica de Catalunya (UPC-Barcelona)
Tel.: + 34 93 401 74 37, fax: + 34 93 401 19 89
E-mail: syurish@sensorsportal.com

Online Registration:

http://www.sensorsportal.com/HTML/SSSD_Course_2008.htm

Deadline for Registration:

31 October, 2008



www.sensorsportal.com